

IOTA 1G

USER MANUAL

Top Client

Data	Average bps	Max bps
2.98 GB	107.53 kbps	2.42 Mbps
489.02 MB	243.02 kbps	2.31 Mbps
11.38 MB	113.95 kbps	529.08 kbps
3.57 MB	12.60 kbps	670.73 kbps
1.27 MB	49.24 kbps	57.07 kbps
1.25 MB	49.64 kbps	57.08 kbps
18.72 kB	222.50 bps	288.00 bps
18.36 kB	216.50 bps	288.00 bps
4.05 kB	658.67 bps	1.02 kbps
3.57 kB	988.00 bps	

Server IP

172.28.190.238
10.0.0.10
192.168.1.1
192.168.1.230
10.13.41.195
192.168.1.255
192.168.192.1

Data

Average bps	Max bps
2.01 GB	413.78 kbps
974.08 MB	101.46 kbps
506.54 MB	121.78 kbps
615.83 kB	71.40 kbps
51.51 kB	17.41 kbps
21.54 kB	340.32 bps
1.84 kbps	7.18 kbps
	176.00 bps
	1.02 kbps



PROFITAP

www.profitap.com

*BRINGING CLARITY INTO NETWORKS.
ANYTIME. ANYWHERE.*

If you have any questions, you can contact us through our website:

[*www.profitap.com*](http://www.profitap.com)

or by email:

[*support@profitap.com*](mailto:support@profitap.com)

For the latest documentation and software, visit our Resource Center:

[*https://www.profitap.com/resource-center/*](https://www.profitap.com/resource-center/)

TABLE OF CONTENTS

1. Product Overview 1

1.1 Hardware Overview	1
1.2 Specifications	2
1.3 Interfaces & LED Behavior	3

2. Getting Started 5

2.1 Deploying the IOTA	5
2.2 Powering the device	7
2.3 Access IOTA over network	7
2.4 IOTA Configuration	9
System Time	9
System Network	10
Access / Internal Firewall	10
ZeroTier	11
System Control	11
System Updates	12

3. Capture Guide 13

3.1 Capture Control	13
3.2 Interface Configuration	15
Port Control	15
Port Status	15
Capture Features	16
Firmware	17
3.3 Autonomous Capture	17

3.4 Data Vault	18
Captured Files	18
Import a PCAP-NG	18
3.5 Data Management	19
Disk Usage	19
Schedule a Cleanup	19
Manual Disk cleanup	20

4. Analysis Guide

21

4.1 Dashboard overview	21
4.2 Basic Navigation	22
Main dashboard selection menu	22
Time range selection	23
Filtering traffic	24
Graphs	25
4.3 PCAP file download	26

5. Legal

28

PRODUCT OVERVIEW

1.1 HARDWARE OVERVIEW

IOTA is a multifunctional passive network probe with integrated traffic capture and analysis capabilities. Designed as a secure and flexible analysis solution, IOTA is a great asset to get access and visibility into industrial or enterprise level networks.

Profitap IOTA is used by network engineers and IT analysts to get a fast and clear overview of the network traffic. This means a comprehensive analysis can be performed quickly, helping engineers get to the root cause in a matter of clicks.

The device can be deployed as a dedicated probe, or programmed for autonomous analysis, eliminating the need of an on-site network expert.




1.2 SPECIFICATIONS

IN-LINE MODE		Yes
IN-LINE LATENCY		1G: 380 ± 8 ns 100M: 720 ± 24 ns 10M: 7600 ± 25 ns
IN-LINE JITTER		20 ns
DUAL SPAN INPUTS MODE		Yes
FAIL-SAFE		Yes
CAPTURE PERFORMANCE		3.2 Gbps / 3.2 Mpps
PACKET PROCESSOR		Yes, 2 Gbps / 3.2 Mpps
HARDWARE TIMESTAMPING		Yes: 8 ns, NTP synchronized
INTERNAL STORAGE		1 TB
POWER INPUTS	12V MODEL	12 VDC
		PoE (management RJ45)
	24V MODEL	24–48 VDC
		PoE (management RJ45)
POWER CONSUMPTION		12 W
MANAGEMENT	Interfaces	10/100/1000 Ethernet
		2 x USB 3.0
	Services	HTTPS (server), UPnP/VPN

1.3 INTERFACES & LED BEHAVIOR

IOTA 1G Interface

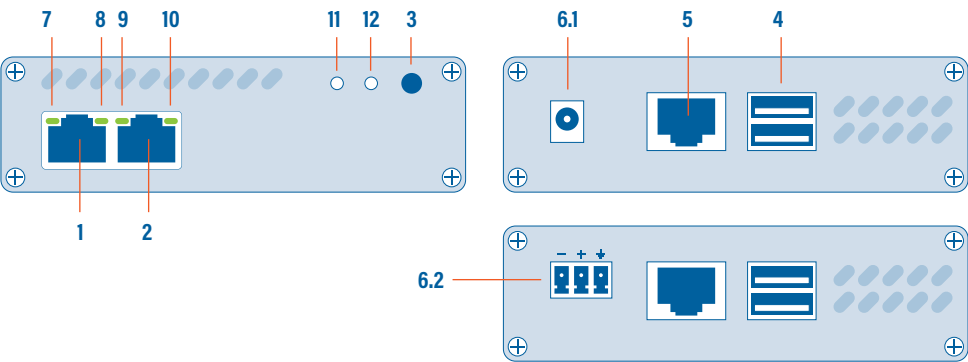

- 1, 2 Ethernet port A, B

3 START/STOP/RESET button

4 2 x USB 3.0 port type A
- 5 RJ45 Management port (PoE)


6.1 12 VDC power input


6.2 24-48 VDC power input

7, 8, 9, 10, 11, 12 Activity LEDs

IOTA 1G LED Behavior

LEDs	STATE	MEANING
	7 and/or 10 steady green	The port is linked.
	7 and/or 10 blinking green	The port is linked and has RX/TX activity (traffic is passing through).
	8 steady green 9 off	Capture interface operating at 10 Mbps speed.
	8 blinking green 9 off	Capture interface is initializing.
	8 off 9 steady green	Capture interface operating at 100 Mbps speed.
	8 off 9 blinking green	Capture interface firmware is corrupted.

LEDs	STATE	MEANING
	8+9 steady green	Capture interface operating at 1 Gbps speed.
	8+9 blinking green	The port is linked and has RX/TX activity (traffic is passing through).
	8+9 alternating blinking	Capture interface cannot find a common speed between the connected devices.

LEDs	LED 11 STATE	LED 12 STATE	MEANING
	Orange Blink	OFF	Booting
	Green	Green	Running
	Green	Green Blink	Capturing
	Green	Orange Blink	Capturing warning
	Green	Red	Disk Full
	Orange Green Blink	Orange Green Blink	Updating
	Red Blink	Red Blink	Hardware Failure
	Orange Blink	Orange Blink	Factory Reset
	Green Blink	OFF	Shutting down
	OFF	OFF	Shutdown completed


GETTING STARTED

2.1 DEPLOYING THE IOTA

IOTA 1G

Insert Ethernet cables of the line you want to monitor into the RJ45 port A and B of the IOTA, using category 5 UTP cables, rated for Gigabit operations.

- **Note:** When deploying IOTA in-line, connect it to the network prior to powering it in order to make full use of its fail-safe capabilities. This step is critical to verify the availability of the in-line path in case of failover.

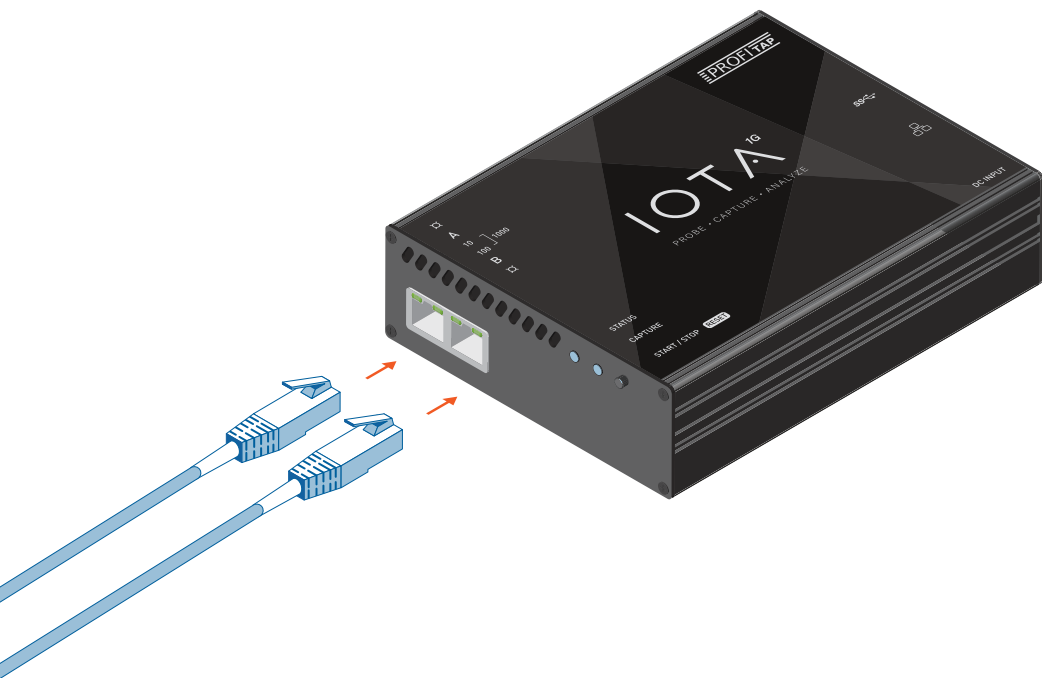

IOTA 1G RACKMOUNT MODEL

The rackmount model can be mounted in a standard 19" rack, using the Profitap Rackmount Chassis Kit (sold separately; reference: ARKB-1U). Secure the chassis to the rack using the provided screws, then insert the IOTA and secure it to the chassis using the thumbscrews on the front panel of the device.



2.2 POWERING THE DEVICE

Connect the 12V/2.5A DC power supply, or the 24–48VDC terminal block, depending on the IOTA model. Alternatively, the device can be powered via PoE, over the management port. Connect both power port and PoE management port for redundant powering, ensuring continued operation in case either port were to be disconnected or unable to provide power.

IOTA boots automatically after a power connection is established. Its status can be observed via the activity LEDs.

- **Note:** Initial boot may take some time to complete. When both the Status and Capture LEDs are green, IOTA has completed the boot sequence.

Once powered, the in-line failover circuit is disabled, effectively placing the device in-line.

2.3 ACCESS IOTA OVER NETWORK

To access the IOTA over the network, connect to the HTTPS interface by browsing to the device IP of your IOTA, including port number.

The full URL should be: `https://x.x.x.x:3000`



DHCP mode is enabled by default. If no IP is assigned to the IOTA, the default fallback IP is **169.254.1.1**.

For the initial login, use the following credentials:

Default username: **admin**

Default password: **admin**

- **Note:** In case your browser displays a 'Your connection is not private' warning, click on **advanced > proceed to...** URL at the bottom to proceed to the IOTA login page.

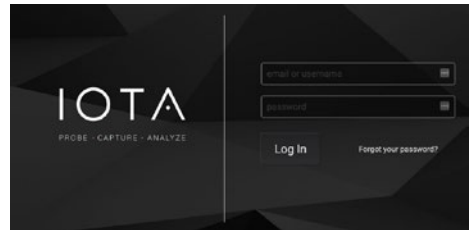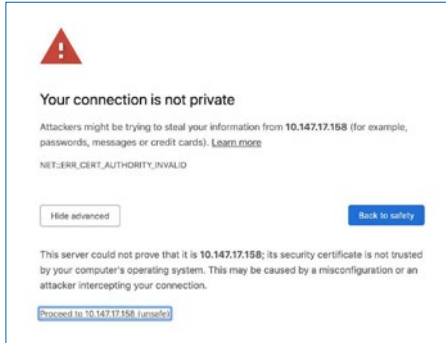

2.4 IOTA CONFIGURATION


System Time

NTP service is enabled by default: if Internet access is provided to IOTA, no extra configuration is required. System time can also be adjusted manually.

The system time is used by:

- the embedded OS,
- the capture interface to constantly discipline the hardware timestamp counter.

Changing time may require a restart of the capture interface to take effect.

 System Time

Date & Time


12/05/2020

15:09


Time Zone

UTC


Apply

 NTP Configuration

Service




Servers



Apply

System Network

Navigate to IOTA Settings / Configuration to change default network settings like IP, Mask, Gateway, DNS and Host Name.

 System Network

Method

DHCP Dynamic

IP

192.168.1.20

Mask

255.255.255.0

Gateway

192.168.1.1

DNS


192.168.1.242

Host Name

iota_d063b401cb2a

Access / Internal Firewall

Used to limit access from local clients (LAN subnetwork) and/or remote clients (WAN, ZeroTier).

 Access

Check to allow

Local access

☒


Remote access

☒

ZeroTier

ZeroTier provides an easy way to remotely access the device via a P2P VPN and manage virtual networks on a cloud application.


(more information: www.zerotier.com)

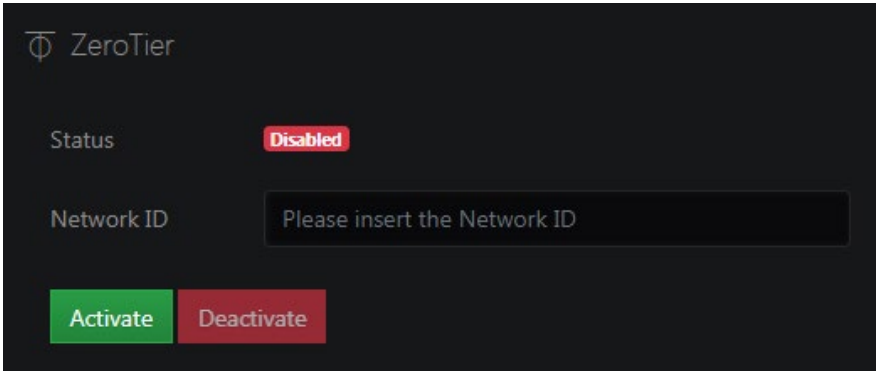

System Control & Logs

Remotely restart or turn off your IOTA by pressing the 'Restart' or 'Shutdown' button.

Download system logs and application logs by pressing the 'System Logs' or 'Application Logs' button.

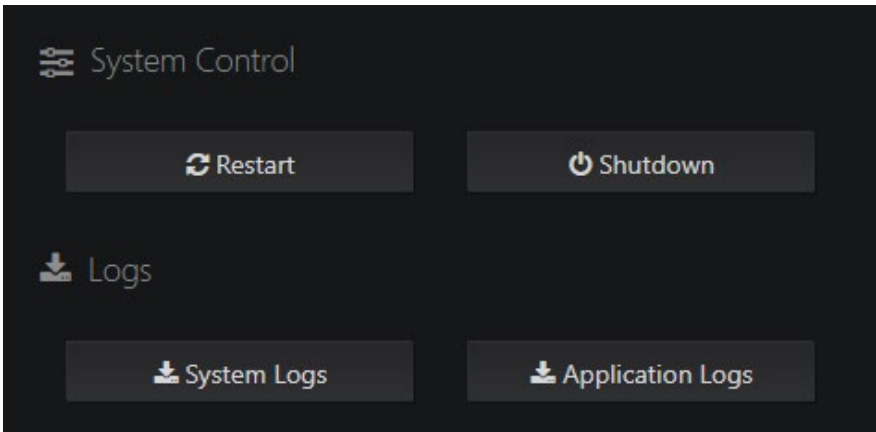

System Updates

The ***IOTA Settings > System Updates*** page provides information about the current IOTA software version, latest available version, and changelog. If the IOTA can access the internet, the latest version number and changelog are fetched automatically, and the IOTA software can be updated via the 'Update' button. If the device cannot access the internet, the latest IOTA software can be downloaded from ***<https://iota.profitap.com/>*** and updated via the 'Select a file' button.

CAPTURE GUIDE

3.1 CAPTURE CONTROL

The interface in **Capture > Capture Control** contains options for the capture of traffic and indexing of captured traffic.

When a capture is in progress, the traffic is automatically indexed in the specified datasource. If the 'Keep Files' option is enabled in the capture interface's settings, the captured traffic is saved on the disk, with new files being automatically created either every 30 seconds, or when the current file's size reaches 4 GB.

- **Note:** Capture files are automatically analyzed and indexed. The 'keep file' option determines whether or not the trace files are conserved in the data vault after having been analyzed.

If the 'keep file' option is enabled, it will be possible to retrieve the complete trace file, part of it, or a filtered copy, from the dashboards.

If the 'keep file' option is disabled, the dashboards will only display the indexed data, and it will not be possible to retrieve the original trace file.

The *Indexing* section defines the database and the index in which the captured data will be indexed.

The default datasource is the database already present on the IOTA device. Other datasources can be selected if they have been set up in **Configuration > Data Sources**.

The *Index* subsection defines which index the captured data will be saved to. Either select an index already present on the selected database, or create a new one by selecting the second option and typing a name (must start with 'profisight').

Edit ProfShark



Nickname profishark_80_0b

Interface Name profishark_80_0b

Device Model IOTA 10G

Device MAC 80:1f:12:3a:02:0b

Keep Files



Close

Apply

Packet Analyzer Settings

DNS Resolution



Indexing

Select a valid Datasource

Elasticsearch - localhost - Default



Index



Select a index



profisight-23.6.2020

Session Keyword



profisight

Files will be available only after the first 30 seconds of capture.

Start Capturing Session

Stop Capturing Session


3.2 INTERFACE CONFIGURATION

The **Capture > Interface Configuration** screen gives an overview of connected devices, Capture Statistics and Device information. To change interface settings, several tabs are available:

Port Control

If IOTA is intended to be used in-line, the appropriate configuration must be set. ‘In-Line mode’ is the default mode (‘Span Mode’ checkbox unticked). IOTA can be set to SPAN Mode by ticking the ‘Span Mode’ checkbox.

Port speed and behavior can be set on this screen, for both port A and port B.

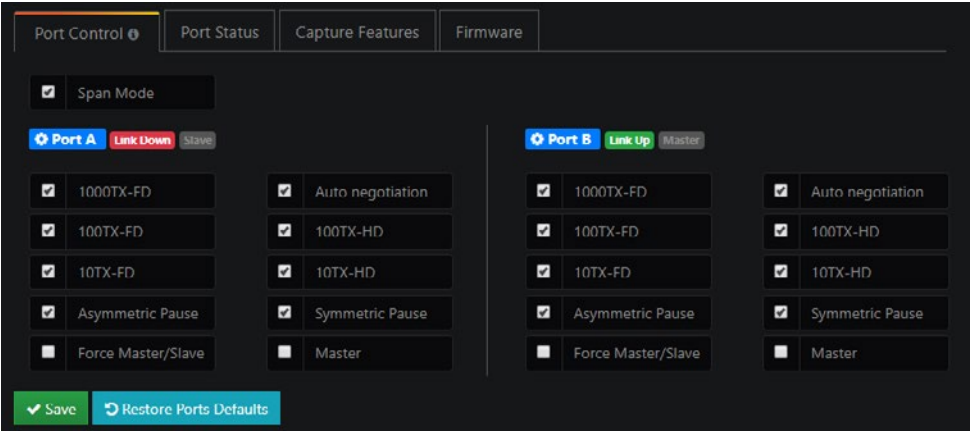

Port Status

This tab provides an overview of the Link Partner Status and Fault Status for both port A and B.

Port Control

Port Status

Capture Features

Firmware

Link Partner Status

A

B

Link Partner Auto-Neg Capable

Yes

Yes

Next Page Request

Yes

Yes

Link Partner Next Page Capable

Yes

Yes

Link Partner Acknowledge Capable

Yes

Yes

Link Partner Advertise 1000BASET_FDX

Yes

Yes

Link Partner Advertise 1000BASET_HDX

No

No

Link Partner Advertise 100BASEIX_FDX

Yes

Yes

Link Partner Advertise 100BASETX_HDX

Yes

Yes

Link Partner Advertise 10BASET_FDX

Yes

Yes

Link Partner Advertise 10BASET_HDX

Yes

Yes

Link Partner Advertise Asymmetric Pause

No

No

Link Partner Advertise Symmetric Pause

No

Yes

Fault Status

A

B

Parallel Decetion Fault

No

No

Remote Fault

No

No

Master/Slave Fault

No

No

Local Receiver Fault

Yes

Yes

Remote Receiver Fault

Yes

Yes

Idle Entry Count

0

0

100BASEIX Lock Error

No

No

100BASETX Receive Error

No

No

100BASEIX Transmit Error

No

No

100BASETX SSD Error

No

No

100BASEIX ESD Error

No

No

1000BASET Lock Error

No

No

1000BASET Receive Error

No

No

1000BASETX Transmit Error

No

No

1000BASEIX SSD Error

No

No

1000BASETX FSD Error

No

No

1000BASETX Carrier Extension Error

No

No

Capture Features

Port Control			Port Status			Capture Features			Firmware		
<input type="checkbox"/> Keep CRC32			<input type="checkbox"/> Disable Port A			<input type="checkbox"/> Disable Port B					
<input type="checkbox"/> Transmit CRC Errors			<input checked="" type="checkbox"/> Packet Slicing (128 bytes)								
<input checked="" type="button" value="Save"/>											


This tab allows the configuration of the following capture settings:

- Transmit CRC Errors
- Keep CRC32
- Packet Slicing (128 bytes)
- Disable Port A
- Disable Port B

Features can be enabled and disabled by ticking or unticking the related checkbox.


Firmware

The firmware can be flashed by selecting a firmware version from the drop-down menu and clicking the 'Flash Firmware' button.

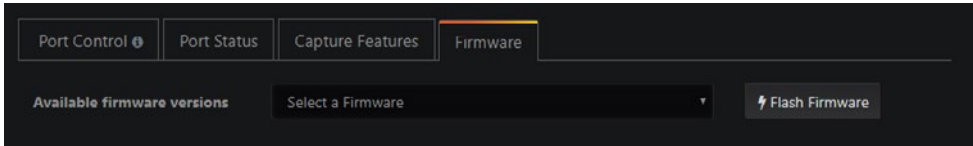

3.3 AUTONOMOUS CAPTURE

To be able to capture traffic in networks where remote access over the network is not allowed or not possible, you can start IOTA's autonomous capture feature by pressing the physical START/STOP button.

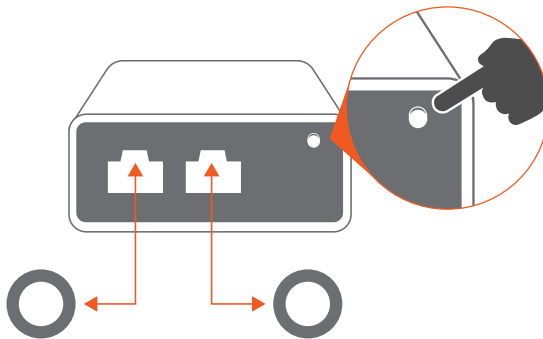

START: Starts capture. IOTA will use latest settings in Capture Control

STOP: Stop Capture

FACTORY RESET: Disconnect power from IOTA. Long-press the START/STOP button and while holding, reconnect power and hold for 20 seconds. FACTORY RESET is complete when LEDs are green.

RESET: Long-press the START/STOP button and hold for 20 seconds. RESET is complete when LEDs are green. This will reset password and network parameters.

SHUTDOWN: Press and hold for 10 seconds for safe device shutdown. This will stop capture and unmount the internal disk in order to end capture session.

- ▶ **Note:** Make sure the appropriate settings have been applied in 'Interface Configuration' before deploying the IOTA in the network you want to analyze.

3.4 DATA VAULT


Captured Files

Navigate to **Data Vault > Captured Files** to download or delete raw PCAP-NG files. Select one or more files and click the 'Download' button to download a .zip archive of the selected files, or the 'Delete' button to delete them.

Q

2015

1 file(s)

<input type="checkbox"/>	Name ⬇	Interface ⬇	Packets ⬇	Filesize ⬇	Created on ⬆
<input checked="" type="checkbox"/>	2015-07-28_mixed.pcapng 	2015-07-28_mixed.pcapng	1437980	876.8 MB	25/07/2015 17:51:36

Delete

Download

Refresh List

page 1 of 1

<

>

Import a PCAP-NG

Importing a PCAP-NG or PCAP file to the IOTA can be done by clicking the 'Select a file' button, selecting the file, and clicking the 'Start Analysis' button. Once uploaded, set the time range of the dashboards to that of the file to ensure the graphs display the correct data.

Use Another Datasource

ProfISight Database - localhost - Default


Index

☐


Select a Index

☒

profisight-24.7.2019

Session Keyword 

profisight

Capture File 

Q Select a file


(up to 10GB)

Start Analysis

3.5 DATA MANAGEMENT

Disk Usage

Navigate to **Data Management > Capture Machine** to get an overview of the disk usage, including total disk size and available disk space.

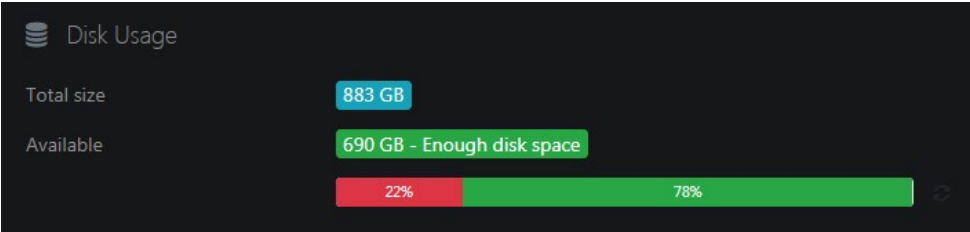

A good practice is to check every once in a while the amount of free storage left and make an assessment on whether a cleanup is in order or not, as there are limitations for capturing and indexing related to the available space:

- New captures can only start if at least 5% of disk space is available.
- Database indexing can only start if at least 10% of disk space is available.
If already running, indexing will stop if less than 10% of disk space remains available.

Schedule a Cleanup

Data retention management is available at **Data Management > Capture Machine > Schedule a Cleanup**. Capture files and index older than the specified time range will be deleted regularly.

The screenshot shows a 'Schedule a Cleanup' form with a dark background. It includes a 'Frequency' input field with the value '2', a unit dropdown menu set to 'Week (s)', and a 'Save Cleanup Event' button. Below the form is a confirmation box stating 'Files older than 2 week(s) will be deleted' with a trash icon.


Frequency: 2 Week (s) Save Cleanup Event

Files older than 2 week(s) will be deleted

Manual Disk Cleanup

Manual cleanup of capture files and index is possible with the following options:

- Selective cleanup based on time
- Selective cleanup based on index
- Cleanup index or PCAP files or both

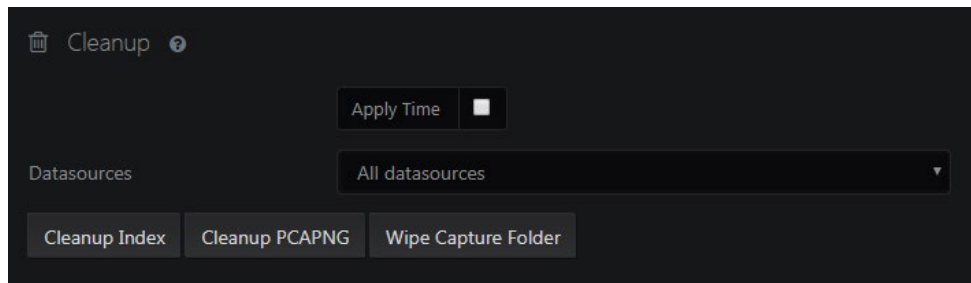

ANALYSIS GUIDE

4.1 DASHBOARD OVERVIEW




1. Main menu
2. Logout
3. Main dashboard selection
4. Time range selection
5. Dashboard area
6. Display filter
7. PCAP file download
8. Dashboard navigation with filters and time selection
9. Dashboard configuration

4.2 BASIC NAVIGATION

Main dashboard selection menu

This menu displays all the available dashboards. The list of dashboards is non-exhaustive and will change over time to include new features and other improvements.

- ▶ **Note:** Accessing a dashboard from this menu resets the Time pickers time range and the Display filter defined in the current dashboard. To navigate through dashboards while keeping the time range and filters set, use the '**Goto >>**' dashboard navigation.

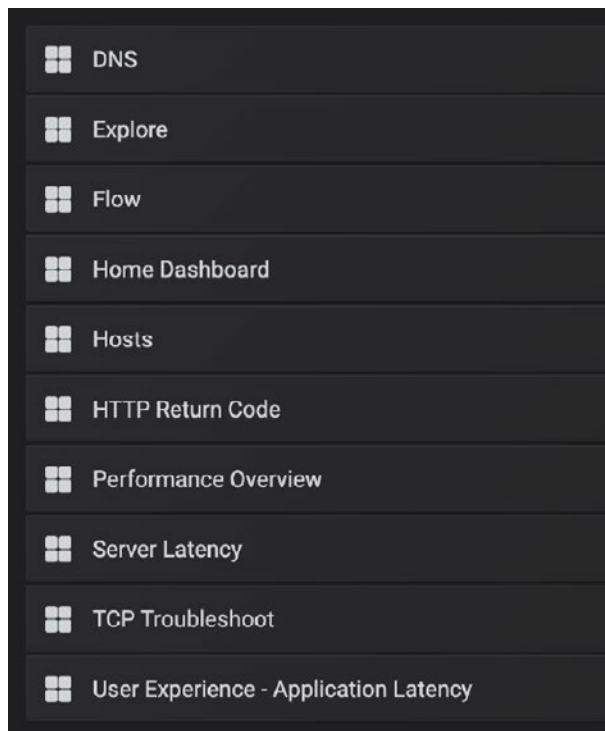

Time range selection

Time range and automatic refresh rate can be set from this menu.

Last 24 hours

Quick ranges

Last 2 days	Yesterday	Today	Last 5 minutes
Last 7 days	Day before yesterday	Today so far	Last 15 minutes
Last 30 days	This day last week	This week	Last 30 minutes
Last 90 days	Previous week	This week so far	Last 1 hour
Last 6 months	Previous month	This month	Last 3 hours
Last 1 year	Previous year	This month so far	Last 6 hours
Last 2 years		This year	Last 12 hours
Last 5 years		This year so far	<u>Last 24 hours</u>

Custom range

From:

now-24h


To:

now


Apply

Filtering traffic


Display filters can be defined manually by clicking the + icon next to the Filter box (top left) and selecting the filter type and value it needs to filter on.

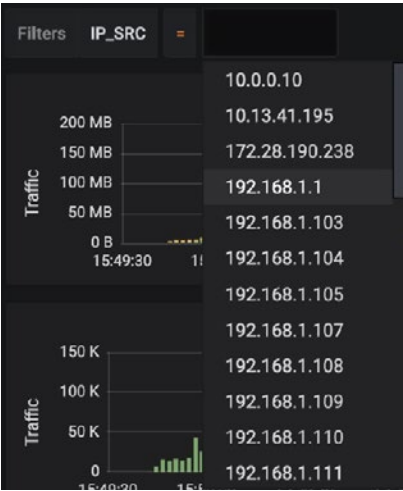

Alternatively, in the dashboards, filters can be applied quickly by using the + magnifier icon (include filter), or the - magnifier icon (exclude filter)

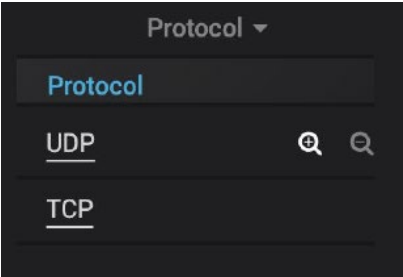


Filters can be removed by clicking the filter type again and selecting '--remove filter--'




Graphs


Click and drag to zoom in on a specific time range.

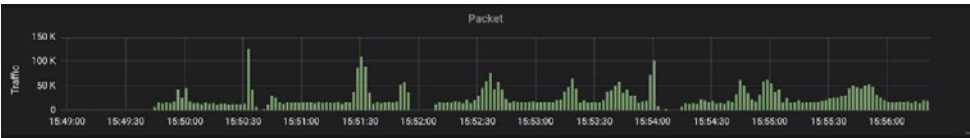

Use CTRL/CMD + mouse drag to add annotations to the graph.

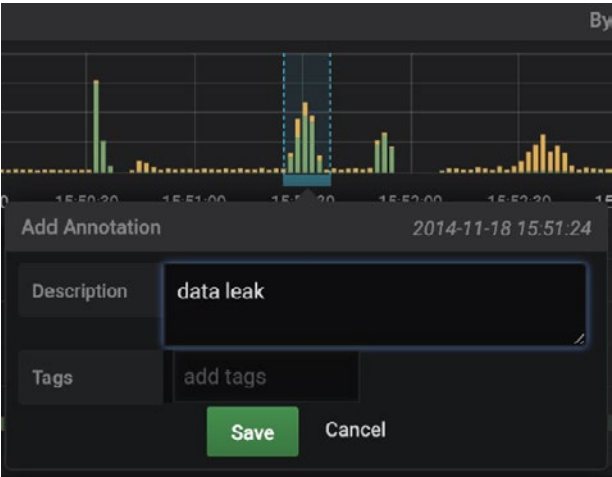

4.3 PCAP FILE DOWNLOAD




Use the 'Get Pcapng' button at the top right corner of any dashboard to download the PCAPNG file.

The time range of the downloaded PCAP file corresponds with the time range selected in the Time picker menu.

The following filters will also apply to the downloaded PCAPNG files:

- ◉ IP address
- ◉ MAC address
- ◉ VLAN ID
- ◉ Protocol
- ◉ Port



If a MAC address, IP address, or port is selected, the filter affects both source and destination.

Additional methods to download PCAP files:

1 - Use the direct download link

Clicking on any link starts the PCAP file transfer, filtered with value only. Filters are ignored with this method.

Top Client ▾				
Client IP		Data ▾	Average bps	Max bps
<u>192.168.1.1</u>	Download PCAP	223.36 MB	89.62 kbps	510.06 kbps
<u>172.28.190.238</u>		15.37 MB	361.52 kbps	2.31 Mbps
<u>192.168.1.241</u>		97.55 kB	44.54 kbps	54.72 kbps
<u>192.168.1.242</u>		82.67 kB	46.54 kbps	54.72 kbps

2 - Download the raw PCAP-NG file(s) from a list

(Data Vault > Captured Files)

The file or group of files are downloaded in a .zip archive.

Q

2015

1 file(s)

Name

↓

Interface

Packets

Filesize

Created on

2015-07-28_mixed.pcapng

2015-07-28_mixed.pcapng

1437980

876.8 MB

25/07/2015 17:51:36

Delete

Download

Refresh List

page 1 of 1

Legal

DISCLAIMER

The manufacturer makes no representations or warranties with respect to the contents hereof and specifically disclaims any implied warranties of merchantability or fitness for any particular purpose. The manufacturer reserves the right to revise this publication and to make changes in the content thereof without obligation of the manufacturer to notify any person of such revision or changes.

COPYRIGHT

This publication, including all photographs and illustrations, is protected under international copyright laws, with all rights reserved. Neither this manual, nor any of the material contained herein, may be reproduced without written consent of the author.

TRADEMARKS

The trademarks mentioned in this manual are the sole property of their owners.

*BRINGING CLARITY
INTO NETWORKS,
ANYTIME,
ANYWHERE.*

PROFITAP HQ B.V. — High Tech Campus 9
5656 AE Eindhoven — The Netherlands

sales@profitap.com
www.profitap.com

© 2020 Profitap — v2.5-07

